

CERTIFICATE OF CALIBRATION no R01538

Customer OREGON STATE UNIVERSITY
Oceanic & Atmos. Sciences
130 Burt Hall
Corvallis OR 97331
USA

Item PTU Transmitter
Pressure range from 500 to 1100 hPa abs., calibrated from 500 to 1100 hPa
Temperature range from - 40 to + 60 °C, calibrated at + 23 °C
Humidity range from 0 to 100 %RH, calibrated from 0 to 97 %RH at + 23 °C

Manufacturer Vaisala Oyj


Model PTU307

Serial number C2610001

Instrument number - -

Calibration performed From July 2 to 4, 2008

Date July 7, 2008

Signature 
Ville Vuorio
Calibration Engineer

Page 1 (11)

Documents attached -

NOTES

This Certificate may only be reproduced in full, except with the prior written permission by the issuing Laboratory.
The measurement results issued in this Certificate are traceable to national or international measurement standards either via ISO/IEC 17025 Accredited Laboratories and/or internal calibrations performed in Vaisala Measurement Standards Laboratory.

Configuration The transmitter's configuration and settings were read from the transmitter's memory. The calibration is valid only with configuration and settings given in table 1.

Table 1. Configuration and settings

Software	PTU300 / 4.02	Fixed P comp.	OFF
Serial number	C2610001	P1 offset	0
Batch number	C2430029	P1 multi adj.	ON
Module 1	AOUT-1	P1 linear adj.	ON
Module 2	BARO-1	P1 poly adj.	OFF
P1 serial num.	C1720020	P1 meas per sec	1 s
Ch3 serial num.	C2310051	P1 average	1 s
EXT factor	0,03	Mlim	512
Filter	OFF	Ta	ON
Pressure	1013.25 hPa		
P comp.	ON		

PRESSURE CALIBRATION

Description The pressure calibration was done in the Measurement Standards Laboratory (MSL) of Vaisala Oyj on July 2, 2008 by Ville Vuorio. Before measurements the transmitter was allowed to stabilize to the conditions of the laboratory for at least 2 hours with + 15,0 VDC \pm 0,3 VDC power supply switched on. Before the calibration the Multi Point Correction (MPC) and Linear Correction (LC) -values for the transmitter were read from the transmitter's memory. The pressure readings of the transmitter were compared to the values of the reference pressure transmitter in the range from 500 to 1100 hPa absolute pressure. Pressure readings of the transmitter were read with the MPC -corrections ON and the LC -corrections OFF. The pressure reading P was then calculated using the old LC -corrections. New LC -corrections were calculated using the least squares method, input into the memory of the transmitter and the final results were calculated using these new corrections. The pressure calibration is valid only with the LC corrections switched ON. Pressure values were read via serial port with resolution of 0,01 hPa. The used pressure transmitting medium was air and/or nitrogen.

Reference DHI PPC3 Pressure Controller/Calibrator, serial number 722, traceable to the National Institute of Standards and Technology (NIST, USA) via MSL and Centre for Metrology and Accreditation (MIKES, Finland).

Uncertainty The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95 %. The standard uncertainty of measurement has been determined in accordance with EA Publication EA-4/02.

- The uncertainty is calculated from the uncertainties caused from the reference equipment, calibration process and unit under calibration (UUC) including resolution, stability (short term), linearity, repeatability, hysteresis and rounding of the final results.
- The measurement results and uncertainty may be interpolated between measurement points.

The measurement uncertainty represents the situation at the time and conditions of calibration. When using the UUC at different conditions and at different time the effect of the conditions and stability of the UUC shall be evaluated separately.



Corrections

The MPC and LC -corrections were read from the transmitter's memory.

Table 2. Multi Point Correction -values

MPC -corrections, P1	
Reading [hPa]	Correction [hPa]
499,60	- 0,09
599,06	- 0,08
698,54	- 0,07
800,93	- 0,06
900,38	- 0,04
999,84	- 0,02
1061,29	- 0,03
1099,33	- 0,04

Table 3. Old Linear Correction -values

Reading	LC -corrections, P1	
0	0,000	[hPa]
0	0,000	[hPa]

Table 4. New Linear Correction -values

Reading	LC -corrections, P1	
500	- 0,047	[hPa]
1100	- 0,007	[hPa]



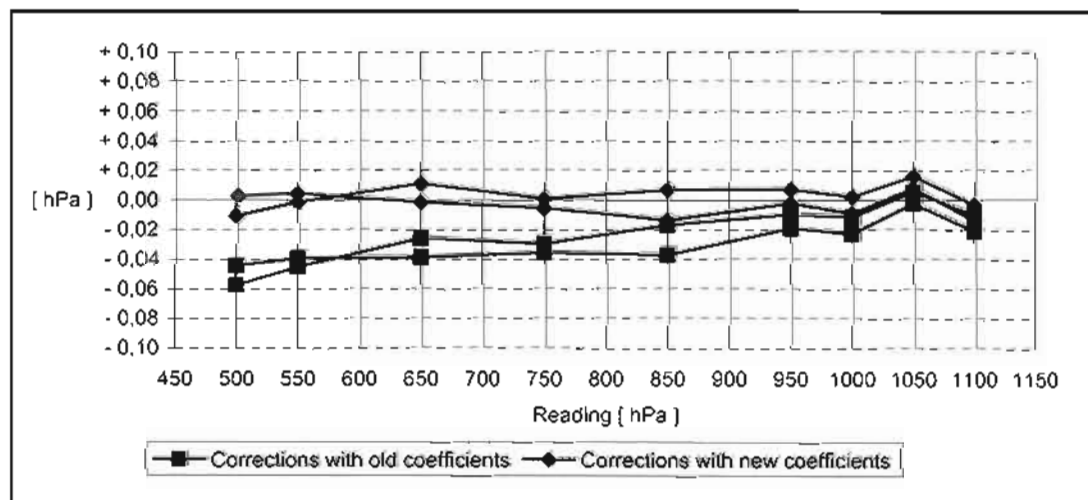
Measurement results

The reference and the reading values presented in table 5 are averages of ten independent observations.

Table 5. Measurement results, pressure

Reference [hPa]	With old coefficients		With new coefficients	
	Reading P [hPa]	Correction [hPa]	Reading P [hPa]	Correction [hPa]
1100,00	1100,02	- 0,02	1100,01	- 0,01
1050,07	1050,07	0,00	1050,06	+ 0,01
999,98	1000,00	- 0,02	999,99	- 0,01
950,05	950,07	- 0,02	950,05	0,00
850,01	850,05	- 0,04	850,02	- 0,01
750,03	750,07	- 0,04	750,04	- 0,01
650,06	650,10	- 0,04	650,06	0,00
550,04	550,08	- 0,04	550,04	0,00
500,07	500,11	- 0,04	500,07	0,00
500,01	500,07	- 0,06	500,02	- 0,01
550,05	550,09	- 0,04	550,05	0,00
650,07	650,10	- 0,03	650,06	+ 0,01
750,06	750,09	- 0,03	750,06	0,00
850,07	850,09	- 0,02	850,06	+ 0,01
950,05	950,06	- 0,01	950,04	+ 0,01
1000,02	1000,03	- 0,01	1000,02	0,00
1050,02	1050,01	+ 0,01	1050,00	+ 0,02
1099,97	1099,98	- 0,01	1099,97	0,00

The correction shall be added algebraically to the reading.


Figure 1. Measurement results

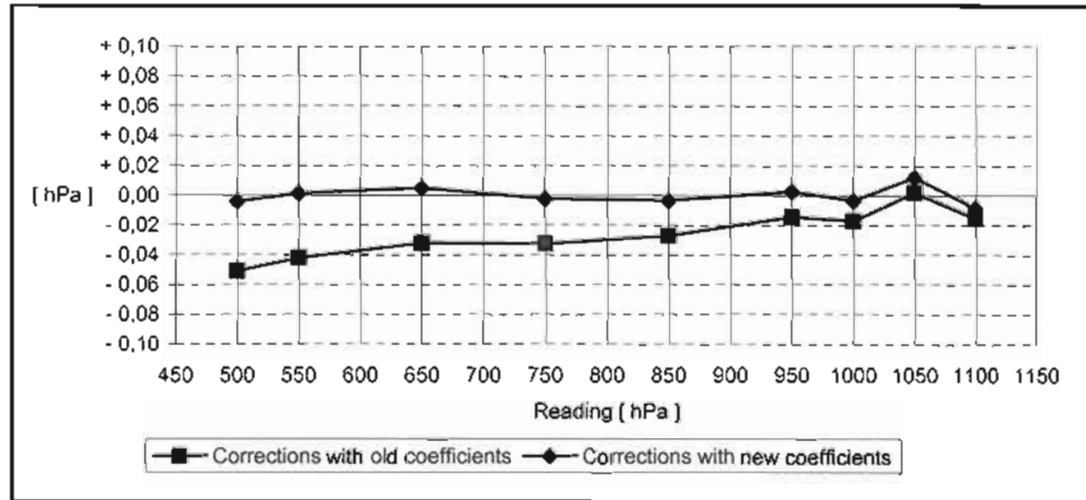

Final results

The reading value is an average of the readings of the pressure transducer installed in the transmitter.

Table 6. Final results, pressure

Reference [hPa]	With old coefficients		With new coefficients		Uncertainty [hPa]
	Reading P [hPa]	Correction [hPa]	Reading P [hPa]	Correction [hPa]	
1099,98	1100,00	- 0,02	1099,99	- 0,01	± 0,08
1050,04	1050,04	0,00	1050,03	+ 0,01	± 0,08
1000,00	1000,02	- 0,02	1000,00	0,00	± 0,08
950,05	950,06	- 0,01	950,05	0,00	± 0,09
850,04	850,07	- 0,03	850,04	0,00	± 0,08
750,04	750,07	- 0,03	750,04	0,00	± 0,08
650,07	650,10	- 0,03	650,07	0,00	± 0,08
550,05	550,09	- 0,04	550,05	0,00	± 0,09
500,04	500,09	- 0,05	500,04	0,00	± 0,09

The correction shall be added algebraically to the reading.


Figure 2. Final results
Conditions

Pressure	1012,4 hPa ± 0,3 hPa
Temperature	+ 23,4 °C ± 0,3 °C
Humidity	39 %RH ± 3 %RH



TEMPERATURE CALIBRATION

Description	<p>The temperature calibration was done in the Measurement Standards Laboratory (MSL) of Vaisala Oyj on July 4, 2008 by Antti Leivonen.</p> <p>Before measurements the transmitter was allowed to stabilize to the conditions of the laboratory for at least 2 hours with + 15,0 VDC \pm 0,3 VDC power supply switched on. The temperature readings of the transmitter were compared to the values of the reference thermometer at 23,0 °C in a calibration chamber.</p> <p>Temperature values were read via serial port with resolution of 0,01 °C.</p> <p>New correction coefficients were calculated and input into the transmitter's memory. Temperature values are given according to the International Temperature Scale of 1990, ITS-90.</p>
Reference	<p>Vaisala PTU200 PTU Transmitter, serial number U0350007, traceable to National Institute of Standards and Technology (NIST, USA) via MSL.</p>
Uncertainty	<p>The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95 %. The standard uncertainty of measurement has been determined in accordance with EA Publication EA-4/02.</p> <ul style="list-style-type: none">- The uncertainty is calculated from the uncertainties caused from the reference equipment, calibration process and unit under calibration (UUC) including resolution, stability (short term), repeatability, self heating and rounding of the final results.- The measurement results and uncertainty are representing the measurement point only. The measurement uncertainty represents the situation at the time and conditions of calibration. When using the UUC at different conditions and at different time the effect of the conditions and stability of the UUC shall be evaluated separately.

Calculations

New offset- and gain coefficients were calculated from the measurement results. The coefficients are presented in table 7. The final results were calculated using equations 1 and 2.

$$T = T \text{ offset} + T \text{ gain} \cdot T', \text{ where} \quad (1)$$

$$T' = \text{Reading without offset- and gain corrections [} ^\circ\text{C]}$$

$$T_a = T_a \text{ offset} + T_a \text{ gain} \cdot T_a', \text{ where} \quad (2)$$

$$T_a' = \text{Reading without offset- and gain corrections [} ^\circ\text{C]}$$

New coefficients were input into the transmitter's memory.

Table 7. Coefficients

	Old coefficients	New coefficients	
T offset	0,000000000000	0,014379999600	[°C]
T gain	1,000000000000	1,000000000000	
Ta offset	0,000000000000	0,015659999800	[°C]
Ta gain	1,000000000000	1,000000000000	

Final temperature results

The reference and the reading values are averages of ten independent observations. The standard deviations are included in the calculated uncertainties.

Table 8. Final temperature results, T

Reference [°C]	With old coefficients		With new coefficients		Uncertainty [°C]
	Reading T [°C]	Correction [°C]	Reading T [°C]	Correction [°C]	
+ 22,99	+ 22,98	+ 0,01	+ 22,99	0,00	± 0,07

The correction must be added algebraically to the reading.

Table 9. Final temperature results, Ta

Reference [°C]	With old coefficients		With new coefficients		Uncertainty [°C]
	Reading Ta [°C]	Correction [°C]	Reading Ta [°C]	Correction [°C]	
+ 22,99	+ 22,97	+ 0,02	+ 22,99	0,00	± 0,07

Conditions

Temperature + 24,1 °C ± 0,3 °C
 Humidity 38 %RH ± 3 %RH

HUMIDITY CALIBRATION

Description	<p>The humidity calibration was done in the Measurement Standards Laboratory (MSL) of Vaisala Oyj on July 4, 2008 by Antti Leivonen.</p> <p>Before measurements the transmitter was allowed to stabilize to the conditions of the laboratory for at least 12 hours with + 15,0 VDC \pm 0,3 VDC power supply switched on. The humidity readings of the transmitter were compared to the reference humidity values at room temperature in Salt Solution Generator in the range from 0 to 97 %RH. The humidity readings were read via serial port with resolution of 0,01 %RH. Coefficients RHI_0, RHI_1, RHI_2, RHI_3 and RHI_4 were calculated from the observed humidity values and input to the transmitter's memory.</p> <p>Measurements were made in Salt Solution Generator, where the temperature was + 23,09 °C \pm 0,03 °C. The 0,1 %RH value was measured in dry nitrogen flow which temperature was + 22,60 °C \pm 0,29 °C.</p>
References	<p>Salt Solution Generator UG 8195, traceability is based on the physical phenomenon in which the equilibrium relative humidity values associated with certain saturated salt solutions are known.</p> <p>The operation principle and values of the Salt Solution Generator are based on Lewis Greenspan's research /1/ and on the international standard ASTM E 104 - 85 /2/.</p>
Uncertainty	<p>The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95 %. The standard uncertainty of measurement has been determined in accordance with EA Publication EA-4/02.</p> <ul style="list-style-type: none">- The uncertainty is calculated from the uncertainties caused from the reference equipment, calibration process and unit under calibration (UUC) including resolution, stability (short term), linearity, repeatability, hysteresis and rounding of the final results.- The measurement results and uncertainty may be interpolated between measurement points. <p>The measurement uncertainty represents the situation at the time and conditions of calibration. When using the UUC at different conditions and at different time the effect of the conditions and stability of the UUC shall be evaluated separately.</p>

Calculations

The new RHI_0 to RHI_4 coefficients were calculated from the measurement results using the least squares method and input into the transmitter's memory.

Complete description of calculations performed is available in the Measurement Standards Laboratory.

During the measurement only temperature T was recorded and the Ta value was calculated using temperature measurement results. With this method the exact humidity readings were calculated with old and new coefficients using equation 3.

$$RH_{OUT} = RH \cdot P_{ws} / P_{wa}, \text{ where} \quad (3)$$

RH = Humidity reading with offset- and gain corrections [%RH]

$$P_{ws} = 6,1078 \cdot 10^{7,5 \left(\frac{T}{T+237,3} \right)} \quad (4)$$

$$P_{wa} = 6,1078 \cdot 10^{7,5 \left(\frac{Ta}{Ta+237,3} \right)} \quad (5)$$

Table 10. Coefficients, humidity

Coefficient	Old coefficients	New coefficients	
RHI_0	0,000000000E+00	+ 1,159999970E-01	[%RH]
RHI_1	0,000000000E+00	- 2,673508880E-02	
RHI_2	0,000000000E+00	+ 4,347300050E-04	[%RH-1]
RHI_3	0,000000000E+00	- 1,399999980E-07	[%RH-2]
RHI_4	0,000000000E+00	0,000000000E+00	[%RH-3]
RH offset	0,000000000E+00	0,000000000E+00	[%RH]
RH gain	1,000000000E+00	1,000000000E+00	

R

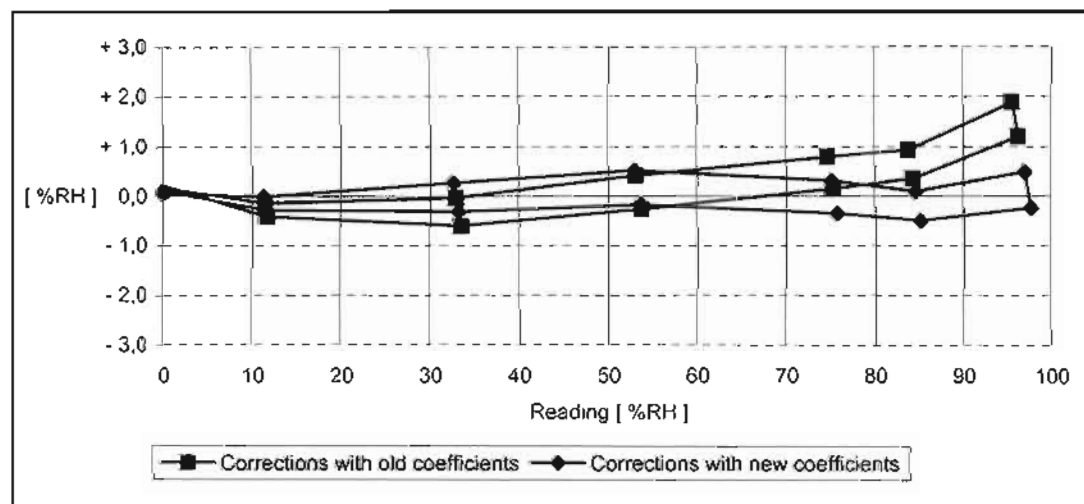
Measurement results

The measurements were made for ascending and descending humidity values. The probe was allowed to stabilize to each humidity for 10 minutes before the reference values were recorded and the humidity and temperature values were recorded ten times. The humidity values were then calculated using the equation 3 and coefficients given in table 10. The calculated humidity values in table 11 are averages of these values.

Table 11. Measurement results, humidity

Reference [%RH]	With old coefficients		With new coefficients	
	Reading RHout [%RH]	Correction [%RH]	Reading RHout [%RH]	Correction [%RH]
0,10	-0,07	+ 0,17	0,04	+ 0,06
11,30	11,44	- 0,14	11,31	- 0,01
32,90	32,94	- 0,04	32,63	+ 0,27
53,47	53,06	+ 0,41	52,95	+ 0,52
75,36	74,57	+ 0,79	75,05	+ 0,31
84,63	83,70	+ 0,93	84,53	+ 0,10
97,41	95,52	+ 1,89	96,92	+ 0,49
97,41	96,21	+ 1,20	97,64	- 0,23
84,63	84,27	+ 0,36	85,13	- 0,50
75,36	75,21	+ 0,15	75,71	- 0,35
53,46	53,72	- 0,26	53,63	- 0,17
32,89	33,50	- 0,61	33,20	- 0,31
11,30	11,72	- 0,42	11,58	- 0,28
0,10	-0,13	+ 0,23	-0,01	+ 0,11

The correction shall be added algebraically to the reading.


Figure 3. Measurement results


Final results

The final humidity calibration results are averages of measured values.

Table 12. Final results, humidity

Reference [%RH]	With old coefficients		With new coefficients		Uncertainty [%RH]
	Reading RHout [%RH]	Correction [%RH]	Reading RHout [%RH]	Correction [%RH]	
0,1	-0,1	+ 0,2	0,0	+ 0,1	± 0,8
11,3	11,6	- 0,3	11,4	- 0,1	± 1,0
32,9	33,2	- 0,3	32,9	0,0	± 0,8
53,5	53,4	+ 0,1	53,3	+ 0,2	± 0,9
75,4	74,9	+ 0,5	75,4	0,0	± 0,8
84,6	84,0	+ 0,6	84,8	- 0,2	± 1,3
97,4	95,9	+ 1,5	97,3	+ 0,1	± 1,6

The correction shall be added algebraically to the reading.

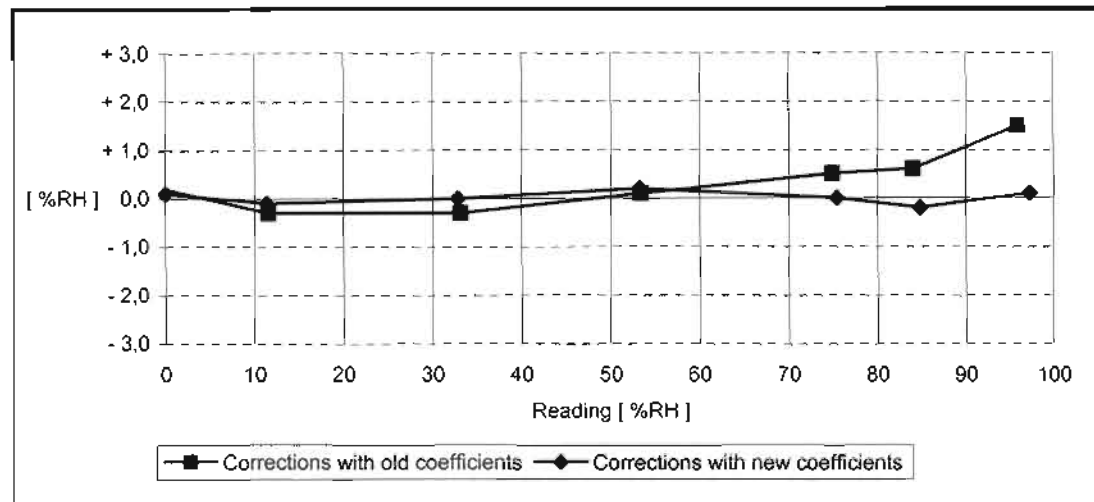


Figure 4. Final results

Conditions
Pressure + 1009,7 °C ± 0,3 hPa
Temperature + 24,1 °C ± 0,3 °C
Humidity 39 %RH ± 3 %RH

REFERENCES

1. Humidity Fixed Points of Binary Saturated Aqueous Solutions. Lewis Greenspan. Journal of Research. Vol. 81A, No. 1, January - February 1977
2. ASTM E 104-85. Standard practice for maintaining constant relative humidity by means of aqueous solutions. ASTM. American Society for Testing and Materials. 1985





Print this order form
 Fill out the required information
 Pack instrument carefully
 Include filled form into the package
 Send to Vaisala

P.O. Box 26, FIN-00421 Helsinki, Finland
 Tel. +358 9 894 91
 Fax. +358 9 8949 2485
 Email: industrialsales@vaisala.com
 www.vaisala.com

Calibration Services for PTU200 and PTU300 Series Transmitters

Please fill in the model(s), serial number(s) and order code with the selected options:

Model (transmitter):	Serial no:											USD
Model (probe, if any):	Serial no:	Code:	X	A					A	A	A	USD
Calibration class	ISO/IEC 17025 Accredited calibration	A										230,-
	ISO 10012 Compliant calibration	B										0,-
Pressure calibration	No calibration	A										0,-
NOTE 1	50, 75, 150, 300, 500, 700, 900, 1000 and 1100 hPa	B										188,-
	500, 550, 650, 750, 850, 950, 1000, 1050 and 1100 hPa	C										188,-
Calibration temperature	+23 °C (room temperature)	A										0,-
Temperature calibration	No calibration/one-point calibration at +23 °C	A										0,-
NOTE 1	0, +20 and +40 °C	B										213,-
	+17.5, +20, +22.5, +25 and +27.5 °C	C										271,-
NOTE 2	-20, 0, +20, +40 and +60 °C	D										271,-
	-35, -20, 0, +20, +40 and +60 °C	E										300,-
	-40, -20, 0, +20, +40 and +60 °C	F										300,-
	0, +10, +20, +30, +40, +50 and +60 °C	G										329,-
Free point 1:	Free point 2:	H										253,-
Humidity calibration	No calibration	A										0,-
NOTE 3	0.1, 11, 33, 53, and 75 %RH	B										194,-
	0.1, 11, 33, 53, 75, 85 and 97 %RH	C										219,-
Adjustment	No adjustment	A										0,-
	Adjusted for optimum performance	B										0,-
Calibration methods	Measurement via serial interface	A										0,-
	Measurement via serial interface and analog outputs (PTU300 series only)	B										100,-
Results reported, pressure	hPa	A										0,-
Results reported, temperature and humidity	%RH and °C	A										0,-
Language of the Certificate	English	A										0,-

NOTE 1: Selected calibration range shall not exceed the measurement range of the transmitter.

NOTE 2: Maximum temperature range of HMP45D probe is from -40 to +60 °C and from -35 to +60 °C for HMP45A/P probe.

Please note that the temperature calibration for the PTU301 transmitter is made at climate chamber with electronics at measurement temperature, all other transmitters are calibrated with electronics at room temperature.

NOTE 3: Please note that the humidity calibration is performed using saturated salt solutions at room temperature.

Please note that one-point temperature calibration at +23 °C temperature is included into the humidity calibration.

Please note that the humidity measurement range in PTU200 does not cover measurement at 0.1 %RH humidity value.

Please fill in the end customer information for Certificate:

End customer	
Order received and approved	



Vaisala Oyj
 P.O.Box 26
 FIN-00421 Helsinki
 Finland
 Tel. (+358 9) 894 91
 Fax. (+358 9) 8949 2227

For other Vaisala
 locations visit us at:
www.vaisala.com