


DOG HOUSE CALIBRATION CHECK

	Set Millivolts	WSD001	DPD001	RSD001	HYD001	AYD001
Record 0	0.0000	0.0853	0.0000	0.0587	-0.0400	0.0600
Record 1	0.1000	0.3307	0.1387	0.3200	0.1280	0.1740
Record 2	1.0000	1.0293	1.2000	1.2000	1.0000	1.0400
Record 3	11.1110	11.4613	11.5787	11.3493	11.0787	11.1267
Record 4	100.0000	100.0160	99.8240	100.0800	99.9400	100.0580
Record 5	100.0000	100.0373	99.8453	100.0800	99.9473	100.0553
Record 6	111.1100	111.0560	111.2160	111.0080	111.0233	111.2253
Record 7	222.2200	222.1067	221.9360	222.0853	222.1660	222.2500
Record 8	333.3300	333.2053	333.4293	333.1520	333.2160	333.3200
Record 9	444.4400	444.3307	443.8293	444.1707	444.2800	444.3947
Record 10	555.5500	555.3600	555.0347	555.3600	555.3653	555.4240
Record 11	666.6600	666.8053	666.3573	666.7733	666.5360	666.6400
Record 12	777.7700	777.5787	777.7493	777.7173	777.5733	777.7573
Record 13	888.8800	888.8107	888.8960	888.5760	888.7013	888.6853
Record 14	999.9900	999.8560	999.7547	999.8027	999.7200	999.9830
Record 15	1111.1100	1111.0610	1110.8160	1110.7310	0.0000	0.0880
Record 16	2222.2200	2221.8030	2221.5470	2221.6530	0.0000	0.0880
Record 17	3333.3300	3332.3090	3332.1390	3332.4800	-0.0120	0.0967
Record 18	4444.4400	4443.4130	4443.1470	4443.6590	-0.0120	0.1000
Record 19	4950.0000	4949.9520	4948.2350	4948.3520	-0.0107	0.0600
Record 20	-4950.0000	-4949.3920	-4948.2530	-4949.0610	-0.0213	0.0600
Record 21	-4444.4400	-4443.9730	-4443.0670	-4443.8190	-0.0113	0.1000
Record 22	-3333.3300	-3333.0400	-3332.2770	-3333.0400	0.0300	0.0567
Record 23	-2222.2200	-2222.1600	-2221.5680	-2221.9200	-0.0280	0.0633
Record 25	-1111.1100	-1111.0030	-1110.7920	-1110.9870	0.0167	0.0647
Record 26	-999.9900	-1000.0110	-999.7760	-1000.0000	-999.8780	-999.7633
Record 27	-888.8800	-888.9600	-888.4800	-888.6933	-888.7467	-888.8027
Record 28	-777.7700	-777.8400	-777.6587	-777.8080	-777.7180	-777.6527
Record 29	-666.6600	-666.8800	-666.3547	-666.6080	-666.5313	-666.5480
Record 30	-555.5500	-555.7067	-555.3280	-555.5200	-555.5067	-555.5260
Record 31	-444.4400	-444.5973	-444.3093	-444.3360	-444.3813	-444.3133
Record 32	-333.3300	-333.5227	-333.0027	-333.1360	-333.2907	-333.2680
Record 33	-222.2200	-222.1600	-222.1120	-222.0533	-222.2040	-222.2167
Record 34	-111.1100	-111.2080	-110.8747	-110.8800	-111.1520	-111.1800
Record 35	-11.1110	-11.1200	-10.9600	-10.8933	-11.0787	-11.0533
Record 36	-1.0000	-0.8133	-0.6640	-0.8560	-0.9447	-0.9400
Record 37	-0.1000	-0.0640	-0.0320	0.0213	-0.0607	-0.0693
Record 38	0.0000	0.0000	0.0907	0.1760	0.0400	0.0567

DOG HOUSE MODULE CHECK

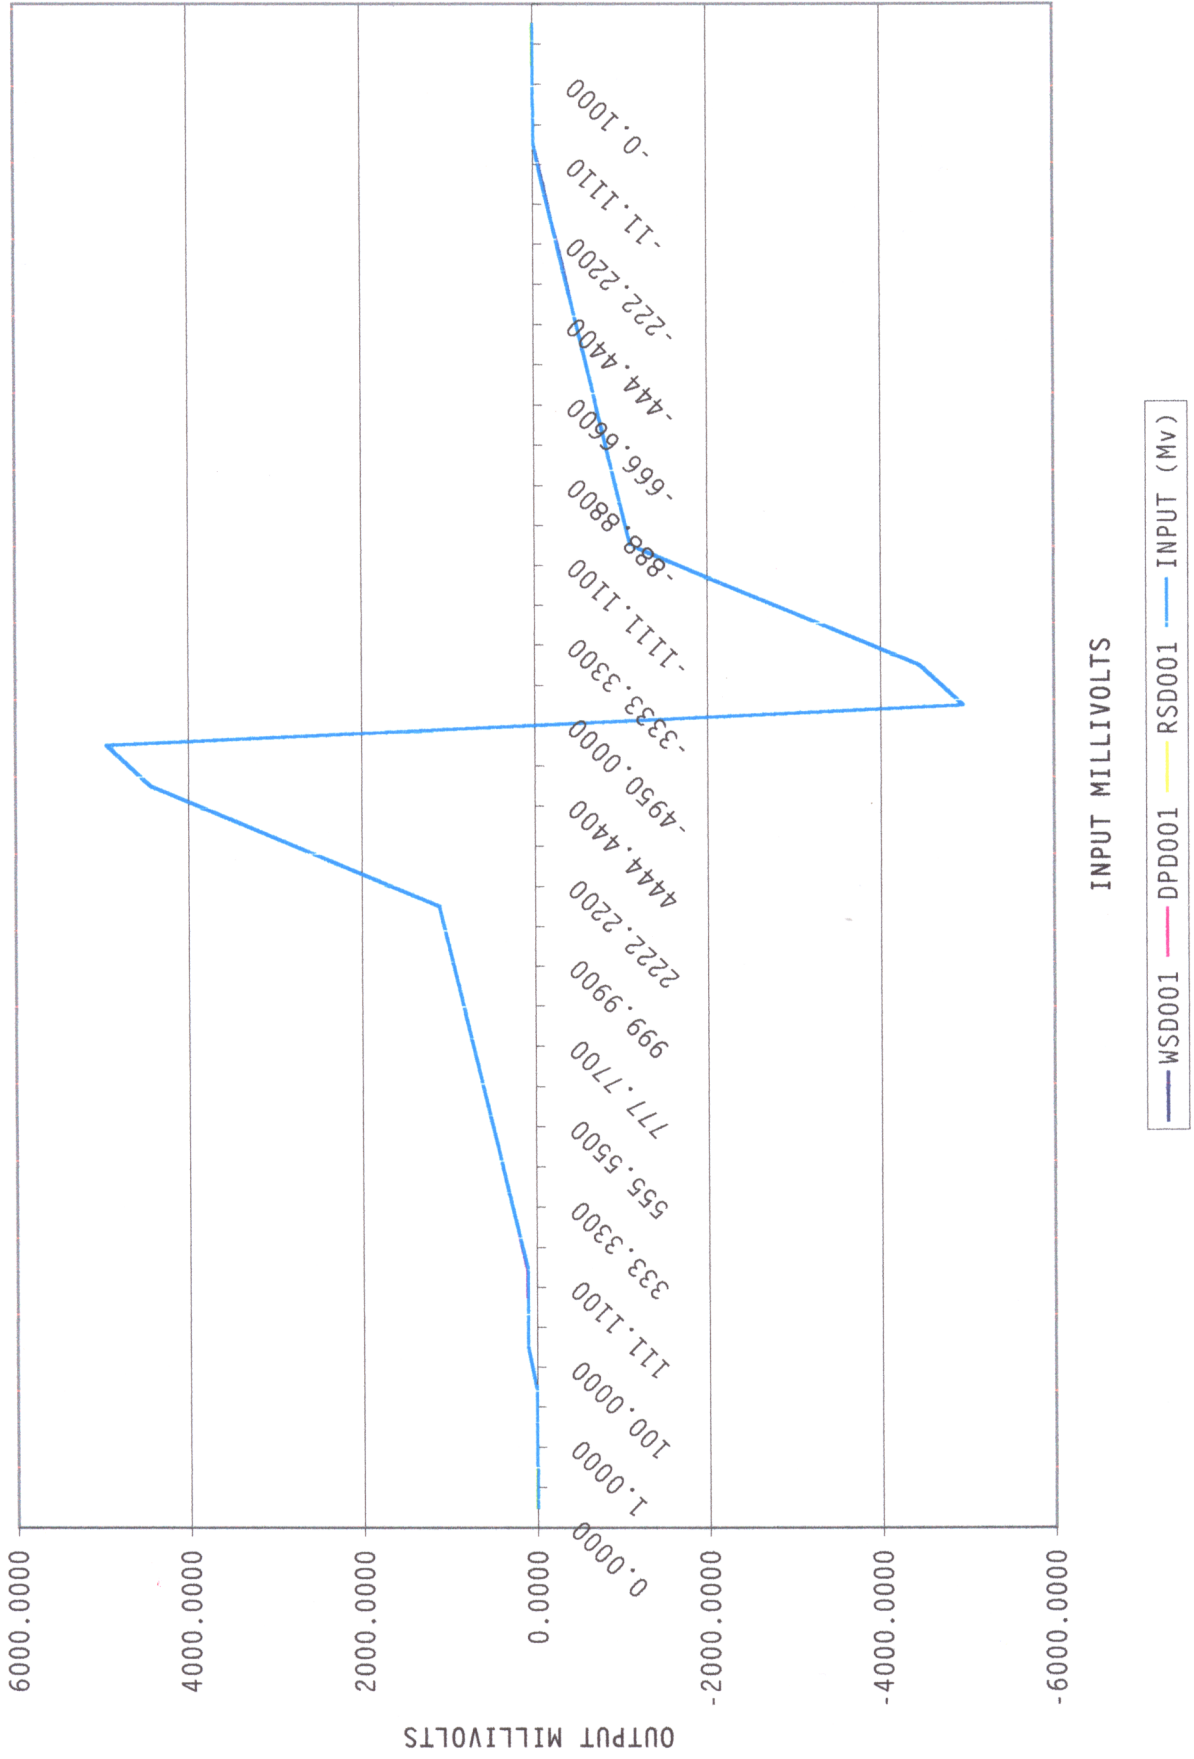

DOG HOUSE MODULE CHECK

