



WET LAB ENCLOSURE MODULE CHECK

	TSF001	CSF001	Input Frequency	Input Voltage	FVB001	SPX001	SPX002	SPX003
Record 0	44.2773	9.9900	10.0000	0.0000	0.0000	0.4480	0.0000	0.0960
Record 1	100.7097	100.7137	100.0000	10.0000	10.0000	10.6453	10.2400	10.2400
Record 2	999.6573	999.6733	1000.0000	100.0000	99.7627	100.2507	100.0693	99.9200
Record 3	1999.8240	1999.8560	2000.0000	1000.0000	999.8613	999.6800	999.6853	1000.1170
Record 4	2998.8320	2998.8590	3000.0000	1111.1100	1110.8590	1110.8800	1110.8160	1111.1470
Record 5	4000.0530	4000.0960	4000.0000	2222.2200	2221.7280	2222.0370	2221.4400	2222.0800
Record 6	5000.4560	5000.4910	5000.0000	3333.3300	3333.1410	3333.3870	3332.1390	3333.1200
Record 7	5999.9250	5999.7970	6000.0000	4444.4400	4443.9570	4443.8930	4442.5170	4444.0530
Record 8	6999.6050	6999.7970	7000.0000	4995.0000	4995.0720	4994.3250	4994.1230	4994.7630
Record 9	8000.0000	8000.0110	8000.0000	-4995.0000	-4996.1390	-4995.3310	-4994.4750	-4995.4530
Record 10	8999.7330	8999.9570	9000.0000	-4444.4400	-4445.0880	-4444.8850	-4444.2610	-4445.0400
Record 11	10000.2880	10000.3200	10000.0000	-3333.3300	-3334.3250	-3333.6960	-3333.2720	-3333.7810
Record 12	10999.3600	10999.3390	11000.0000	-2222.2200	-2223.3970	-2222.8000	-2222.6080	-2223.0560
Record 13	11994.1230	11994.4530	12000.0000	-1111.1100	-1112.5600	-1111.8400	-1111.8400	-1112.0480
Record 14	12983.8720	12984.0110	13000.0000	-1000.0000	-1001.4320	-1000.7360	-1000.7200	-1000.7520
Record 15	13995.5200	13995.6910	14000.0000	-100.0000	-101.2000	-100.7200	-101.0880	-100.8480

FLOW THROUGH MODULE FREQUENCY CHECK

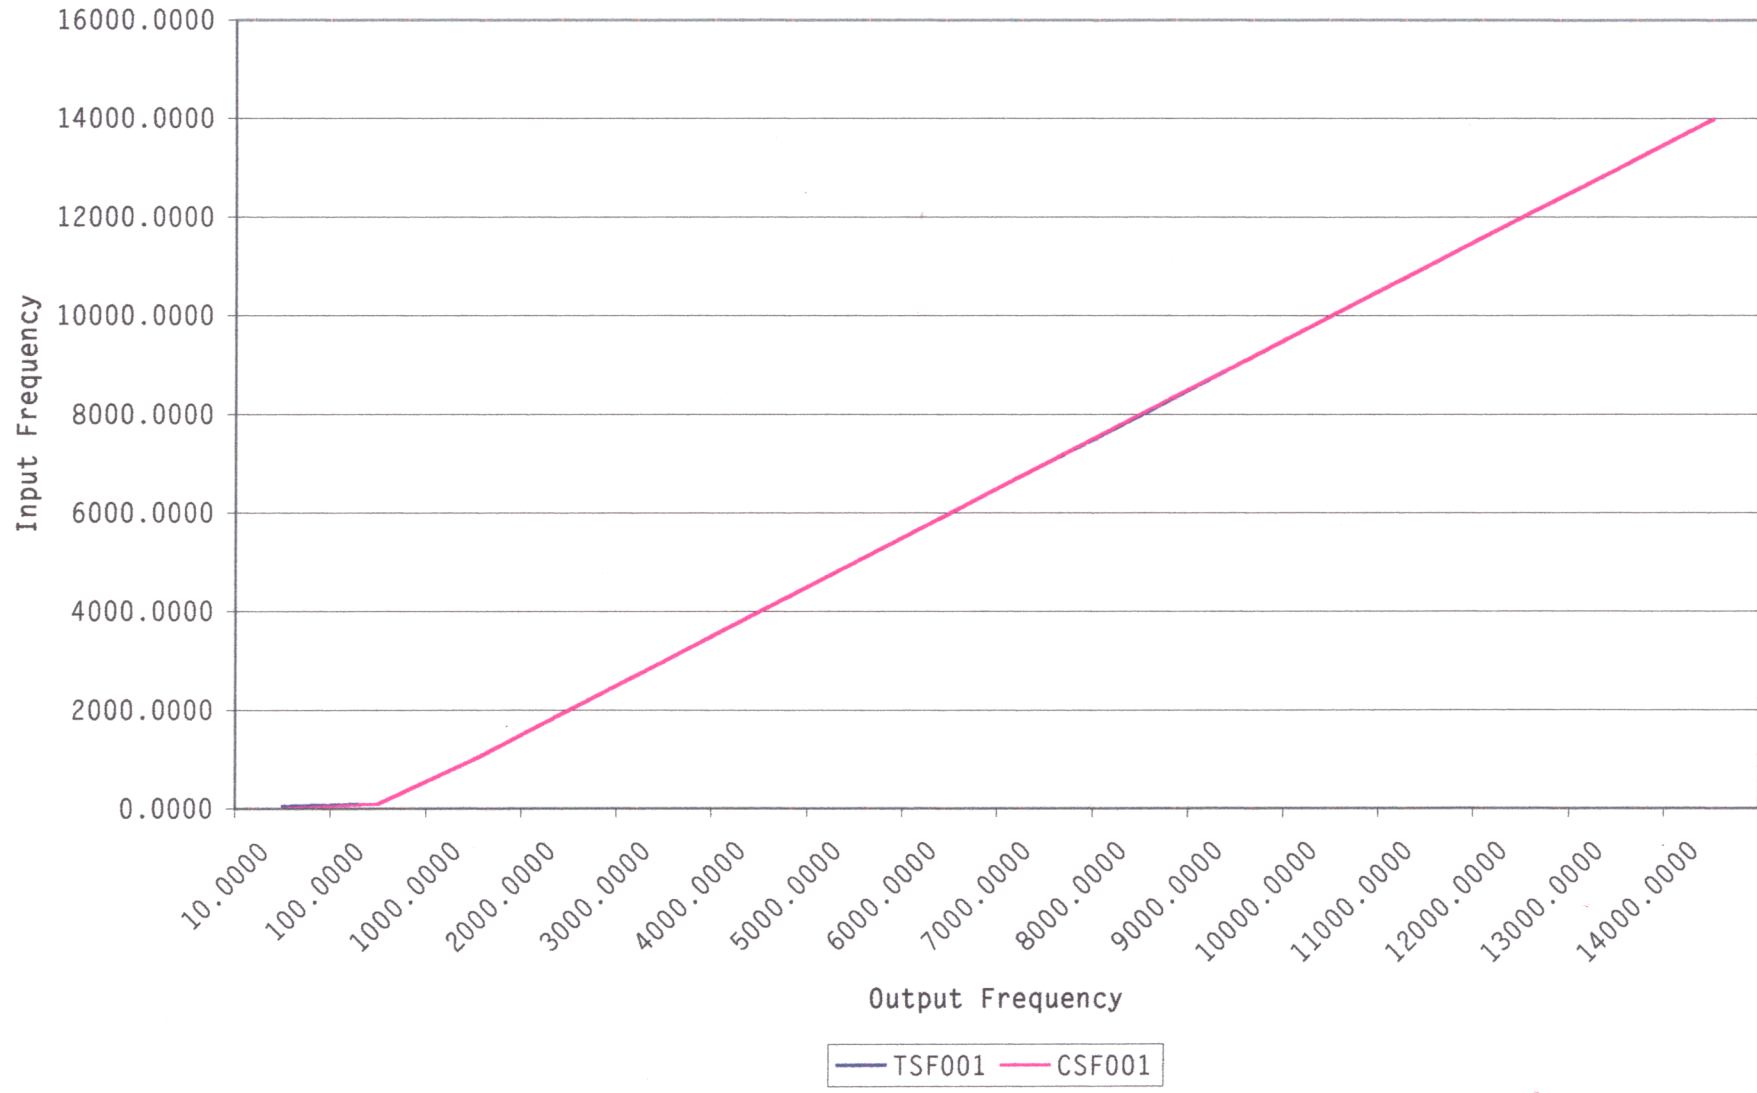

WET LAB ENCLOSURE MODULES CHECK

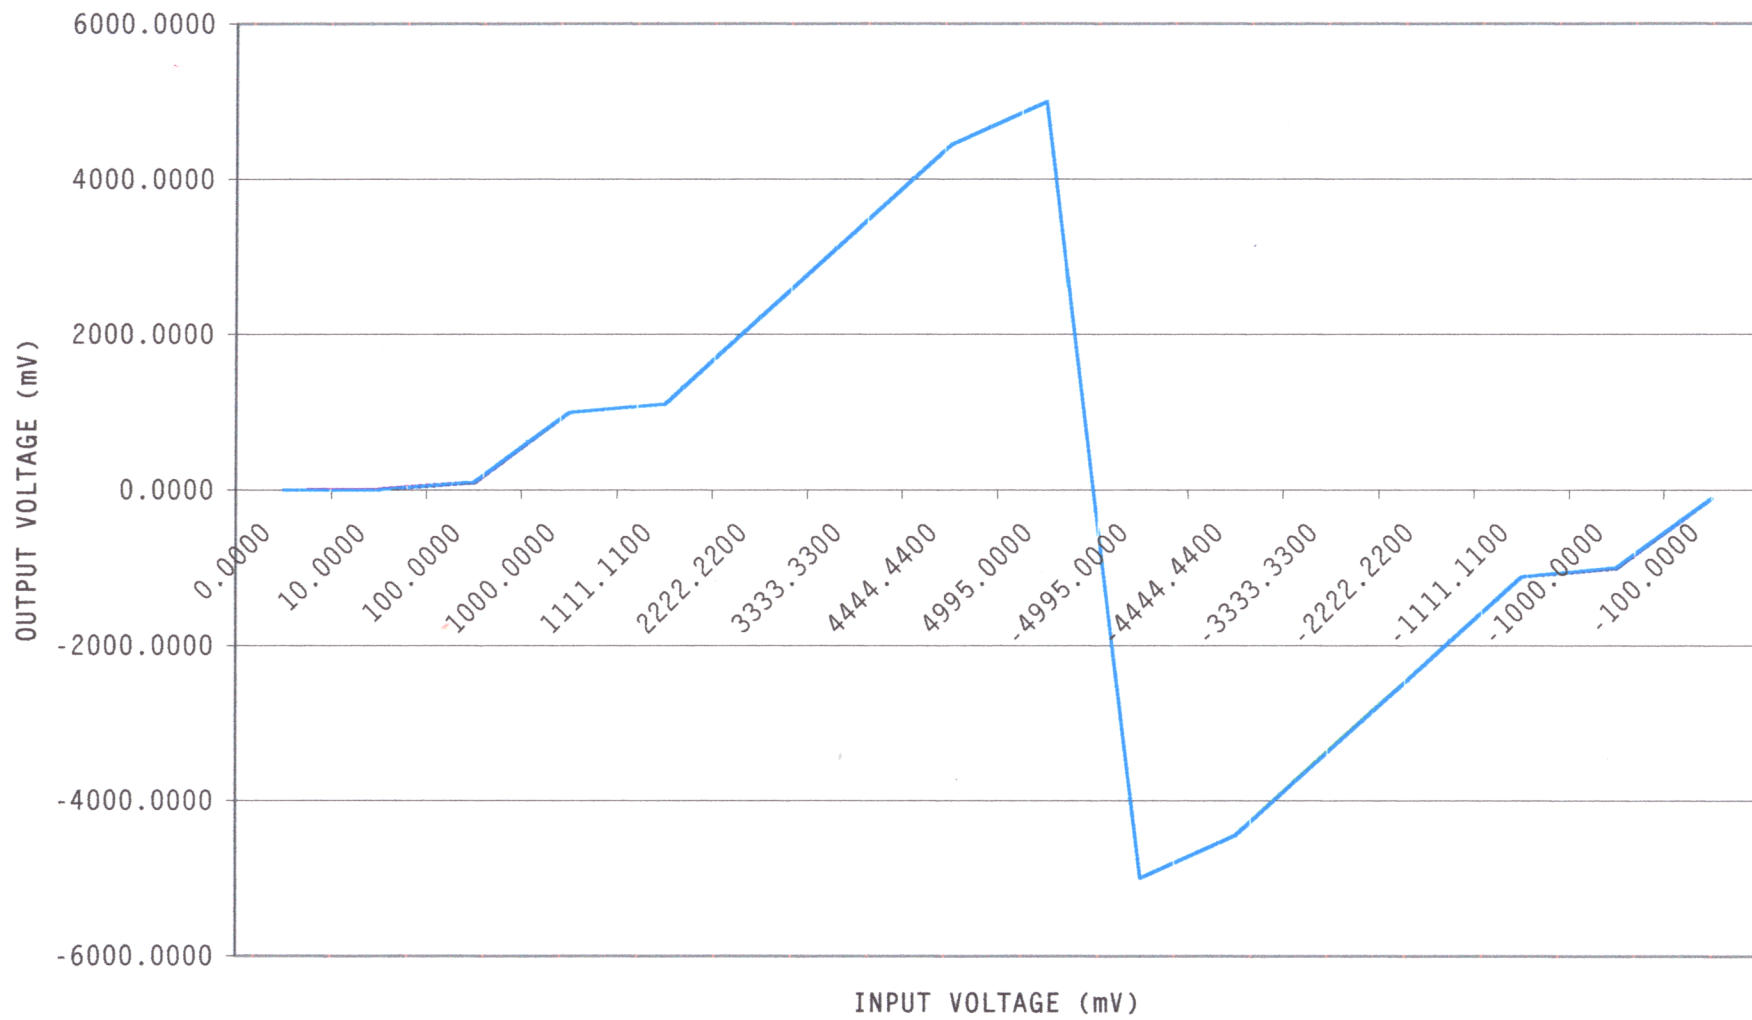

FVB001 SPX001 SPX002 SPX003