

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1041
CALIBRATION DATE: 17-Nov-06

SBE4 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHIJ COEFFICIENTS

g = -4.10472627e+000
h = 5.61249093e-001
i = 1.64285941e-005
j = 3.07787712e-005
CPcor = -9.5700e-008 (nominal)
CTcor = 3.2500e-006 (nominal)

ABCDM COEFFICIENTS

a = 4.07577342e-005
b = 5.61240765e-001
c = -4.10465701e+000
d = -1.11489999e-004
m = 3.9
CPcor = -9.5700e-008 (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.70371	0.00000	0.00000
-0.9971	34.9671	2.81583	7.56913	2.81584	0.00001
14.9999	34.9675	4.28818	9.12784	4.28812	-0.00007
18.4999	34.9652	4.63597	9.45817	4.63603	0.00006
28.9999	34.9619	5.72346	10.42211	5.72347	0.00001
32.4999	34.9577	6.09784	10.73351	6.09783	-0.00001


Conductivity = $(g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p)$ Siemens/meter

Conductivity = $(af^m + bf^2 + c + dt) / [10(1 + \epsilon p)]$ Siemens/meter

t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

Date, Slope Correction

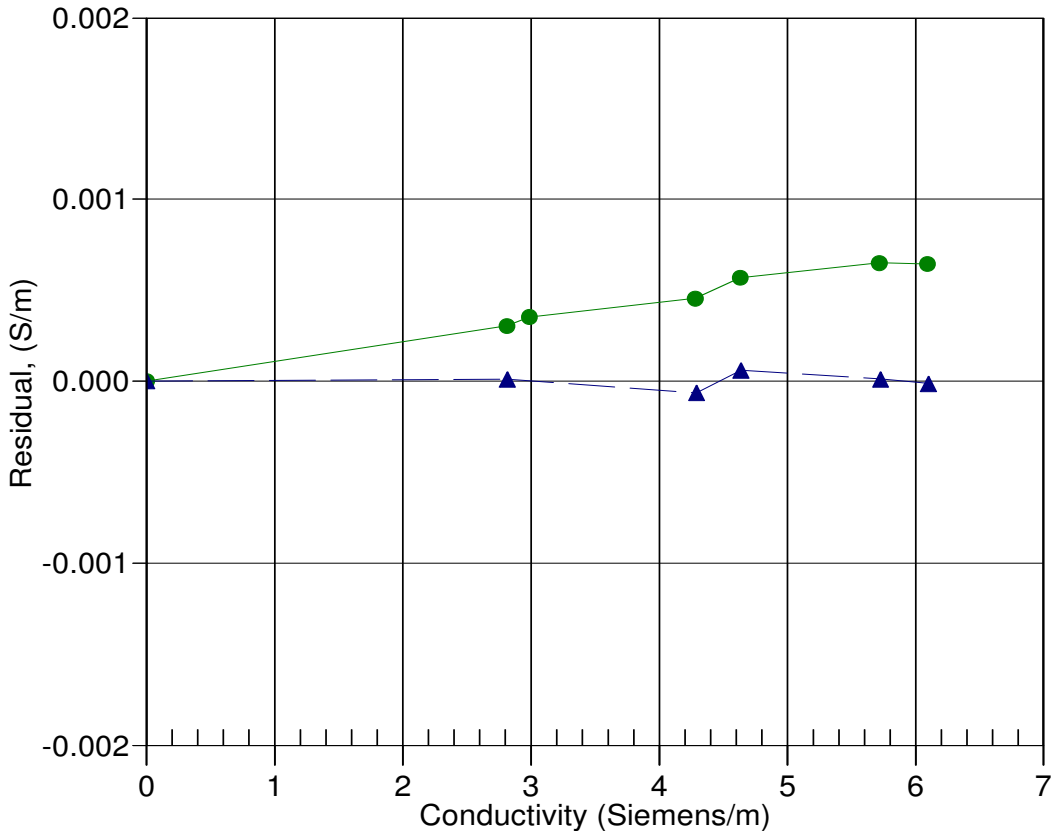

● 16-Sep-05 0.9998885
▲ 17-Nov-06 1.0000000