

SEA-BIRD ELECTRONICS, INC.

13431 NE 20th Street, Bellevue, Washington, 98005-2010 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1568
CALIBRATION DATE: 09-Jun-11

SBE4 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHIJ COEFFICIENTS

g = -4.00515538e+000
h = 5.19008426e-001
i = -1.48750759e-004
j = 3.19141504e-005
CPcor = -9.5700e-008 (nominal)
CTcor = 3.2500e-006 (nominal)

ABCDM COEFFICIENTS

a = 1.04830361e-005
b = 5.18594679e-001
c = -4.00414271e+000
d = -8.64176669e-005
m = 4.3
CPcor = -9.5700e-008 (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.77838	0.00000	0.00000
-1.0000	34.8798	2.80921	7.85797	2.80920	-0.00002
1.0000	34.8801	2.98090	8.06488	2.98093	0.00003
15.0001	34.8814	4.27876	9.48204	4.27875	-0.00001
18.5001	34.8815	4.62609	9.82618	4.62607	-0.00002
29.0001	34.8790	5.71144	10.83014	5.71151	0.00007
32.5000	34.8704	6.08435	11.15369	6.08431	-0.00004


Conductivity = $(g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p)$ Siemens/meter

Conductivity = $(af^m + bf^2 + c + dt) / [10(1 + \epsilon p)]$ Siemens/meter

t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

Date, Slope Correction

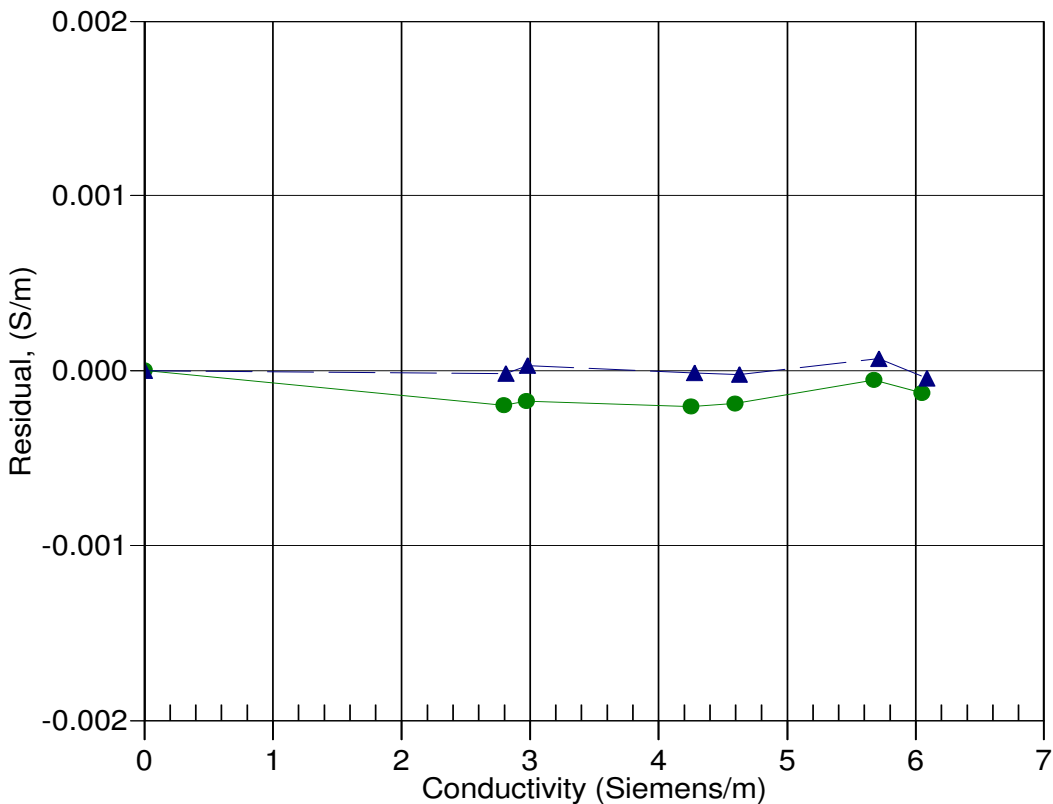

● 28-Jan-10 1.0000311
▲ 09-Jun-11 1.0000000