

SEA-BIRD ELECTRONICS, INC.

13431 NE 20th Street, Bellevue, Washington, 98005-2010 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1898
CALIBRATION DATE: 09-Jun-11

SBE4 CONDUCTIVITY CALIBRATION DATA
PSS 1978: C(35,15,0) = 4.2914 Siemens/meter

GHIJ COEFFICIENTS

g = -1.05873746e+001
h = 1.51802107e+000
i = -3.20654917e-005
j = 8.79659841e-005
CPcor = -9.5700e-008 (nominal)
CTcor = 3.2500e-006 (nominal)

ABCDM COEFFICIENTS

a = 1.02841112e-004
b = 1.51786604e+000
c = -1.05871656e+001
d = -8.45429516e-005
m = 3.9
CPcor = -9.5700e-008 (nominal)

BATH TEMP (ITS-90)	BATH SAL (PSU)	BATH COND (Siemens/m)	INST FREQ (kHz)	INST COND (Siemens/m)	RESIDUAL (Siemens/m)
0.0000	0.0000	0.00000	2.64046	0.00000	0.00000
-1.0000	34.8798	2.80921	5.04433	2.80920	-0.00001
1.0000	34.8801	2.98090	5.15494	2.98092	0.00002
15.0001	34.8814	4.27876	5.92413	4.27876	-0.00000
18.5001	34.8815	4.62609	6.11347	4.62607	-0.00002
29.0001	34.8790	5.71144	6.67039	5.71148	0.00004
32.5000	34.8704	6.08435	6.85117	6.08433	-0.00003


Conductivity = $(g + hf^2 + if^3 + jf^4) / 10(1 + \delta t + \epsilon p)$ Siemens/meter

Conductivity = $(af^m + bf^2 + c + dt) / [10(1 + \epsilon p)]$ Siemens/meter

t = temperature[°C]; p = pressure[decibars]; δ = CTcor; ϵ = CPcor;

Residual = (instrument conductivity - bath conductivity) using g, h, i, j coefficients

Date, Slope Correction

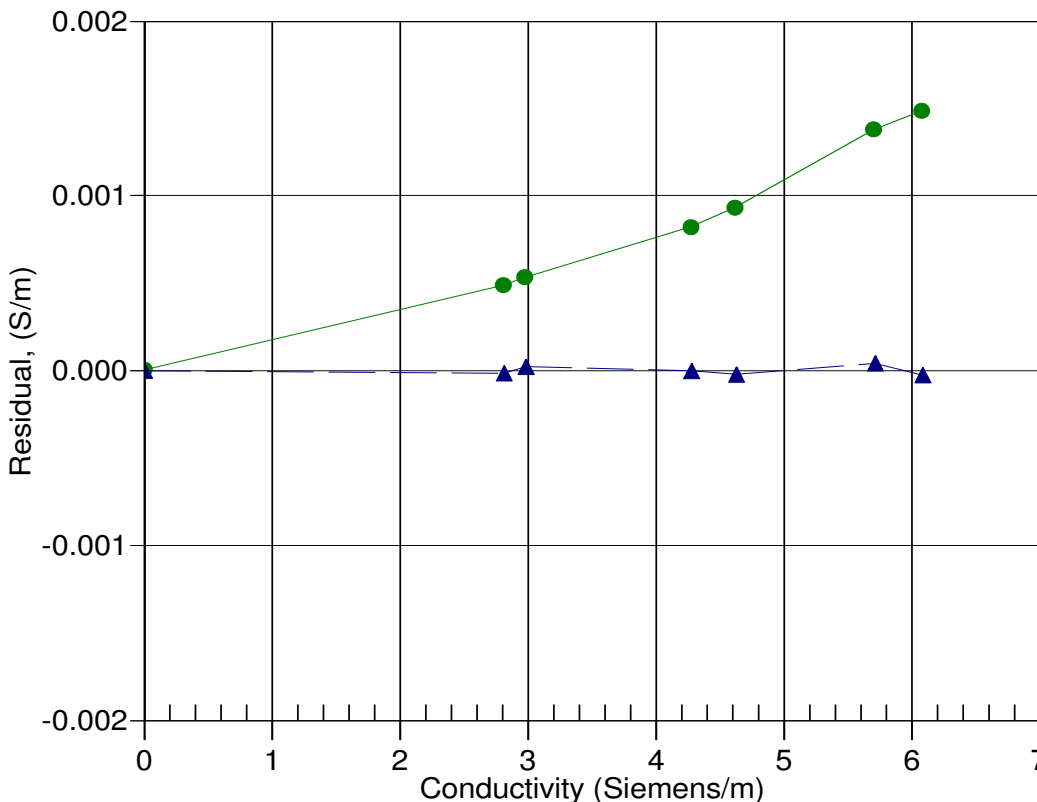

● 04-Nov-09 0.9997802
▲ 09-Jun-11 1.0000000