

SEA-BIRD ELECTRONICS, INC.

1808 136th Place N.E., Bellevue, Washington, 98005 USA

Phone: (425) 643 - 9866 Fax (425) 643 - 9954 Email: seabird@seabird.com

SENSOR SERIAL NUMBER: 1232
CALIBRATION DATE: 09-May-09p

SBE 43 OXYGEN CALIBRATION DATA

COEFFICIENTS

Soc = 0.4074

Voffset = -0.4946

Tau20 = 2.07

A = -9.8225e-005

B = 9.7245e-005

C = -2.3084e-006

E nominal = 0.036

NOMINAL DYNAMIC COEFFICIENTS

D1 = 1.92634e-4 H1 = -3.30000e-2

D2 = -4.64803e-2 H2 = 5.00000e+3

H3 = 1.45000e+3


BATH OX (ml/l)	BATH TEMP ITS-90	BATH SAL PSU	INSTRUMENT OUTPUT(VOLTS)	INSTRUMENT OXYGEN(ml/l)	RESIDUAL (ml/l)
1.24	2.00	0.01	0.808	1.24	-0.00
1.24	6.00	0.01	0.843	1.24	-0.00
1.25	12.00	0.01	0.898	1.25	-0.00
1.26	20.00	0.01	0.971	1.26	-0.00
1.27	26.00	0.02	1.029	1.26	-0.00
1.27	30.00	0.02	1.071	1.27	-0.00
4.12	12.00	0.01	1.826	4.13	0.01
4.13	6.00	0.01	1.656	4.13	0.00
4.13	2.00	0.01	1.543	4.13	0.00
4.13	20.00	0.01	2.061	4.13	0.00
4.14	26.00	0.02	2.247	4.14	0.00
4.15	30.00	0.02	2.377	4.15	-0.00
5.11	30.00	0.02	2.817	5.12	0.00
6.74	26.00	0.02	3.347	6.75	0.00
6.78	20.00	0.01	3.061	6.78	-0.00
6.84	12.00	0.01	2.700	6.84	-0.00
6.91	6.00	0.01	2.437	6.91	-0.00
6.97	2.00	0.01	2.262	6.97	-0.00

$$\text{Oxygen (ml/l)} = \text{Soc} * (\text{V} + \text{Voffset}) * (1.0 + \text{A} * \text{T} + \text{B} * \text{T}^2 + \text{C} * \text{T}^3) * \text{OxSol}(\text{T},\text{S}) * \exp(\text{E} * \text{P} / \text{K})$$

V = voltage output from SBE43, T = temperature [deg C], S = salinity [PSU] K = temperature [deg K]

OxSol(T,S) = oxygen saturation [ml/l], P = pressure [dbar], Residual = instrument oxygen - bath oxygen

Date, Delta Ox (ml/l)

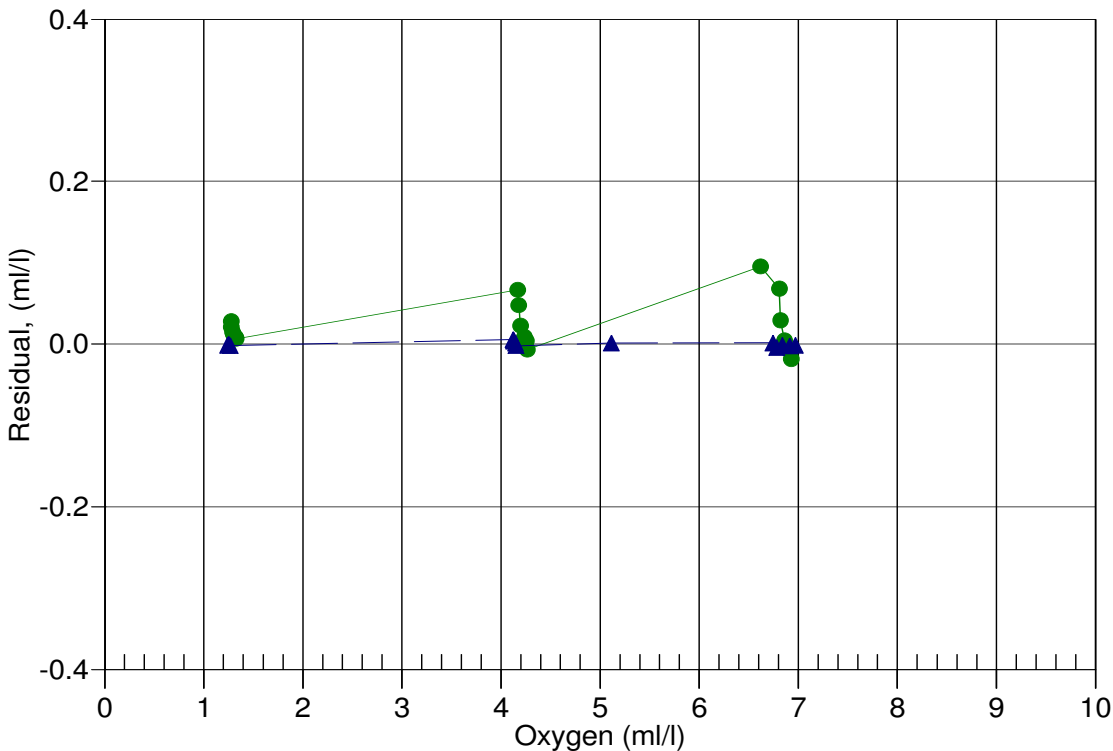

● 24-Oct-08p 0.9953
▲ 09-May-09p 1.0000